





Table of contents

1. Introduction	3
2. Intended use	3
3. tempmate.®-S2 models	4
4. Device description	
5. Display indicators	
6. Quick Start Guide	8
7. Operation and use	10
Configuration	10
Start logger	
Set mark	11
Stop logger	11
Manual readout	11
Readout with tempbase software	12
8. Important notes	13
9. Main Technical Specifications tempmate.®-S2 T	14
10. Main Technical Specifications tempmate.®-S2 TH	15
13. Contact information	16

1. Introduction

The tempmate.®-S2 is designed to be mounted on a broadcast or stationary and measure relevant parameters such as temperature and optionally relative humidity. The device records data and stores it on an internal memory.

2. Intended use

The tempmate.®-S2 is designed to be mounted on shipments or stationary and to record relevant parameters as mentioned in the datasheet. Any use or operation requiring specific requirements and standards not explicitly mentioned in the data sheet must be validated and tested at the customer's responsibility.



3. tempmate.®-S2 models



V1.0-11/2022-EN · Technical Changes and Errors excepted

LCD


Single-use


Temperature

Rel. humidity



4. Device description

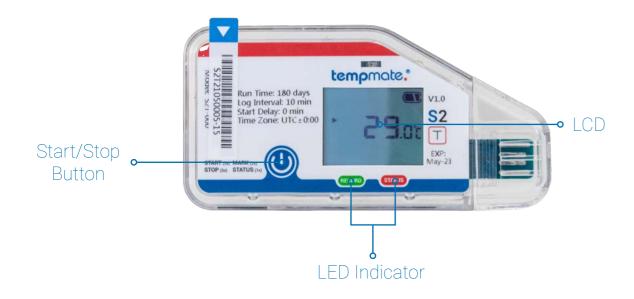

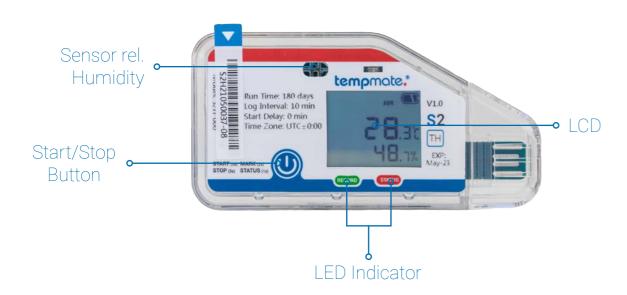

5. Display indicators

Press the Start button repeatedly to call up the individual pages on the device display.



Not started



Started*



Stopped



Number measured values



Highest measured value



Lowest measured value



Average value



MKT



Time & Date

* If the start delay is set, this symbol flashes after a successful start until the time limit has elapsed.



6. Quick Start Guide



























7. Operation and use

STEP 1 Configuration *optional

This step is only necessary if you want to adapt the already pre-installed configuration to your application.

- Download the free tempbase 2 software. https://www.tempmate.com/de/download/
- Install the tempbase 2 software on your PC.
- Remove the cap and connect the not started logger to your PC.
- Open the tempbase 2 software and select the "Logger Setup" button (1).
- Make the desired settings and save them on your device using the "Save Parameter" button (2)
- Remove the logger from your PC and replace the cap securely.



STEP 2 Start logger

- Press and hold the blue button 🔘 for 5 seconds.
- A successful start is indicated by the green LED on your device flashing 10 times.
- <u>Important:</u> If another or no flashing signal appears, do not use the logger and contact support.

STEP 3 Set mark

- Press the blue button twice in succession to set a mark.
- A successfully set marker is indicated by the word "MARK" and the number of markers set so far in your display.
- Important: Up to 10 marks can be set per operation.

STEP 4 Stop logger

- Press and hold the blue button **(()** for 5 seconds.
- A successful stop is indicated by the red LED on your device flashing 10 times.

Alternative stop modes

Automatic stop (default setting)

- The device will stop automatically when the maximum number of readings in the data memory is reached and no manual stop is performed beforehand.
- o This stop mode works in addition to the manual stop...

Software stop (optional)

- o This setting can be made in the tempbase 2 software. (see STEP 1)
- The stop is triggered automatically by connecting the logger to the PC and opening the software.
- A manual stop is not possible in this configuration.

STEP 5 Manual readout


- Remove the cap and connect the logger to your PC.
- A successful connection is indicated by both LEDs flashing. The abbreviations CSV and PDF appear one after the other in the display.



- The logger will automatically open as an external drive on your PC. This process may take a few minutes depending on the amount of data.
- Open the drive and copy the PDF and CSV report stored to a local folder.
- Important: A report is automatically generated as PDF and/or CSV when the device is stopped. The device can still be read out during a running measurement and an intermediate report can be downloaded.

Readout with tempbase 2 software (optional)

- Remove the cap and connect the logger to your PC.
- Open the tempbase 2 software and select the "Export/Import" button (3).

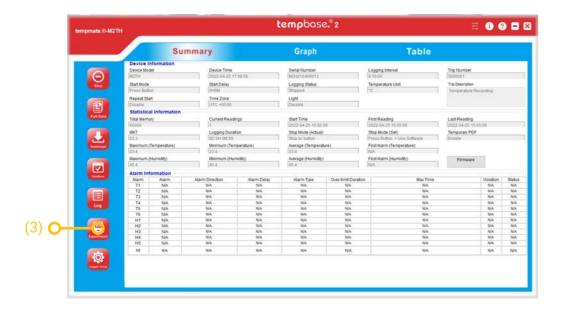

- Select the desired file format (PDF/XLS/IME) for export and the file location and confirm the download.



8. Important notes

- The configuration of your device cannot be changed during recording.
- If you connect the device to the PC without a manual stop, a temporary stop of the recording is triggered. You can now download an interim report. After disconnecting the device from your PC, the recording will continue automatically.
- Always dispose of devices according to your country's regulations.
- Do not place the device in corrosive liquids and do not expose it to direct heat.





Main Technical Specifications **temp**mate.®-S2 T

on cell battery
thers)
Standard Model est
est

Other Specifications

Temporary PDF	The PDF Report is available at any time without stopping the Logger
Software	PDF reader + optional tempbase 2 Software
Reprogrammable	Yes, with optional tempbase 2 Software
Backup-Log-Feature	Yes
Custom ID and Travel Description	Yes
Calibration Certificate	Yes, with 6 points (hardcopy) & PDF in memory
Conformity	EN 12830, CE, RoHS
Serial Number Identification	Yes



Main Technical Specifications **temp**mate.®-S2 TH

Т	L	1	
$\overline{}$			

Recording Options	Single-Use
Dimension [mm]	93 x 47 x 8 mm
Weight [g]	30g
Casing	Ecofriendly Hardcase
Battery	CR2450 lithium metal button cell battery
Connection Interface	USB 2.0, A-Type (integrated)
Display	Multifunction LCD
Protection Class	IP52
Shelf Life	24 months
Temperature Range	−30 °C to 70 °C
Temperature Accuracy	±0.3°C (-20 to 40°C) ±0.5 (others)
Temperature Resolution	0.1 °C
Humidity Range	0 - 100 %rH
Humidity Accuracy	±3%rH (20 to 80%rH) ±5% (others, at 25°C)
Humidity Resolution	0.1 %rH
Ambient Light Sensor	Yes
Memory Capacity (measurements)	32,000 points (T/rH)
Run Time (Logging Interval)	Up to 180 days (10 min.) = Standard Model
	Other models only on request
Data Export	PDF & CSV
Alarm Configuration	up to 5 points temperature and 2 points humidity customizable
Startup Mode	Button
Stop Mode	Button or by Software

Other Specifications

Temporary PDF	The PDF Report is available at any time without stopping the Logger
Software	PDF reader + optional tempbase 2 Software
Reprogrammable	Yes, with optional tempbase 2 Software
Backup-Log-Feature	Yes
Custom ID and Travel Description	Yes
Calibration Certificate	Yes, with 6 points (hardcopy) & PDF in memory
Conformity	EN 12830, CE, RoHS
Serial Number Identification	Yes

Since environmental influences can affect the lifespan of batteries, we recommend that all our products be stored in the conditions that are optimal for them. In this way, the shelf life given at the time of purchase can be guaranteed. Optimal storage conditions: +15°C to +23°C / 45% to 75% rH.

15 V1.0-11/2022-EN · Technical Changes and Errors excepted




Contact information



Do you have any questions? Please contact us - our experienced team will be happy to support you.

sales@tempmate.com

+49 7131 6354 0

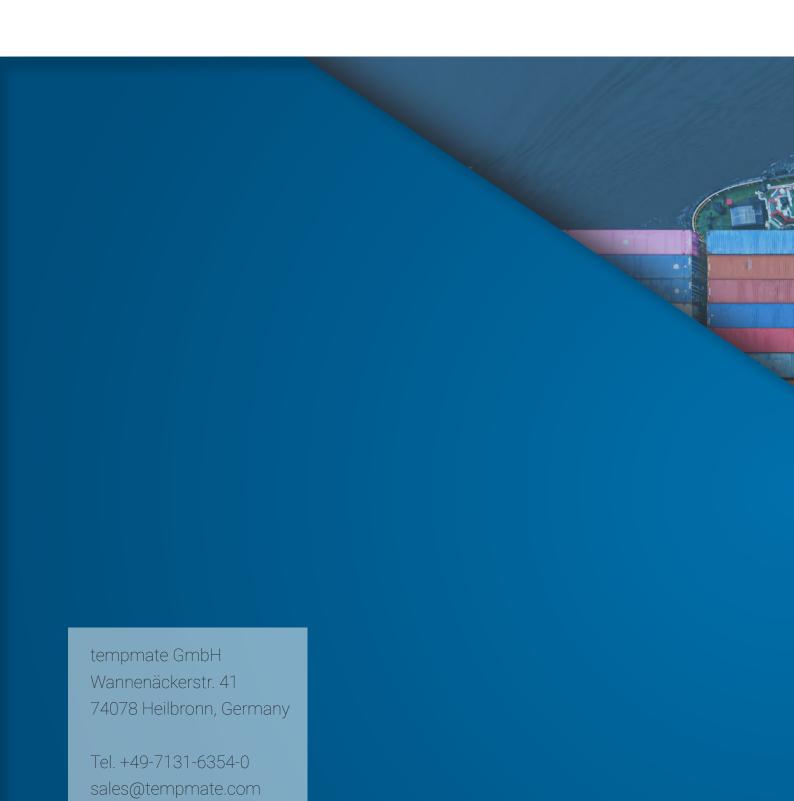

www.tempmate.com